MIDMARK®

Installation Instructions

9A254002 SEAT RAIL ASSEMBLY

KIT COMPONENTS

Part Number	Description	Qty.
9A254002	Seat Rail Assembly	1 pair
• 041-0375-10	3/8"-16 Nut	4
• 040-0375-75	3/8"-16 x 4" hex socket flat head bolt	4
003-1027-00	I / O Instructions	1

REQUIRED TOOLS

9/16" Socket or Wrench
7/32" Allen Wrench
Phillips Screwdriver

INTRODUCTION

To provide a secure, stationary support for attachment of Midmark accessories to seat section of table.

WARNING

Do not install on same side of table that has a 9A27200X Base Rail. Remove any Base Rails before installing the Seat Rail. Multiple attachment of accessories on a single rail is not recommended. Failure to comply may result in personal injury or equipment damage.

INSTALLATION

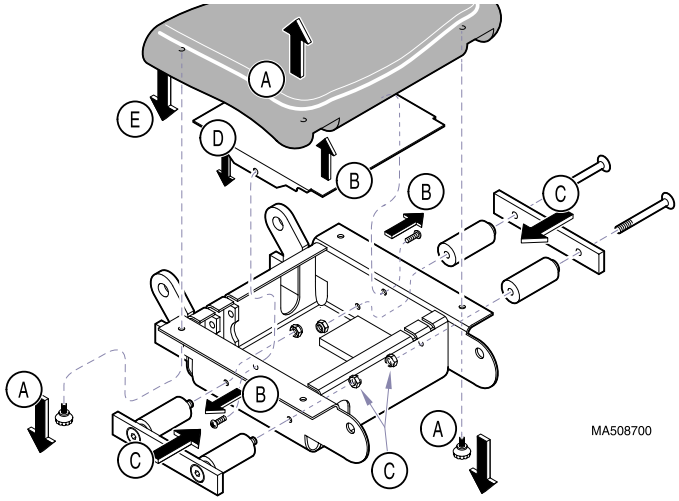

DANGER

Always unplug unit from electrical outlet before removal of any panels or performing any work on unit. Failure to comply could result in personal injury from electrical shock.

NOTE

For ease of installation, place table in a flat position, then unplug table from electrical outlet.

A. Remove the four (4) knobs that secure the seat upholstery to the table and remove the seat upholstery.

B. Remove two (2) screws and remove seat electrical cover.

WARNING

Discharge capacitors where terminals are exposed before performing and work on unit. Failure to comply could result in personal injury from electrical shock.

NOTE

Seat rails are inter-changeable, either can be used on the patient's right or left side.

C. Place seat rails in position and secure with four (4) nuts, 2 per rail.

D. Install seat electrical cover.

E. Install seat upholstery.

© Midmark Corporation - 1999